


Peak Analysis

Injection Details					
Injection Name:	m-4-N3-100g			Run Time (min):	10.67
Vial Number:	149			Injection Volume:	5.00
Injection Type:	Unknown				
Calibration Level:					
Instrument Method:	80 hold 2 min 30 per 280 hold 2 min				
Processing Method:	Qualitative			Dilution Factor:	1.0000
Injection Date/Time:	07/Oct/23 09:48			Sample Weight:	1.0000

Chromatogram

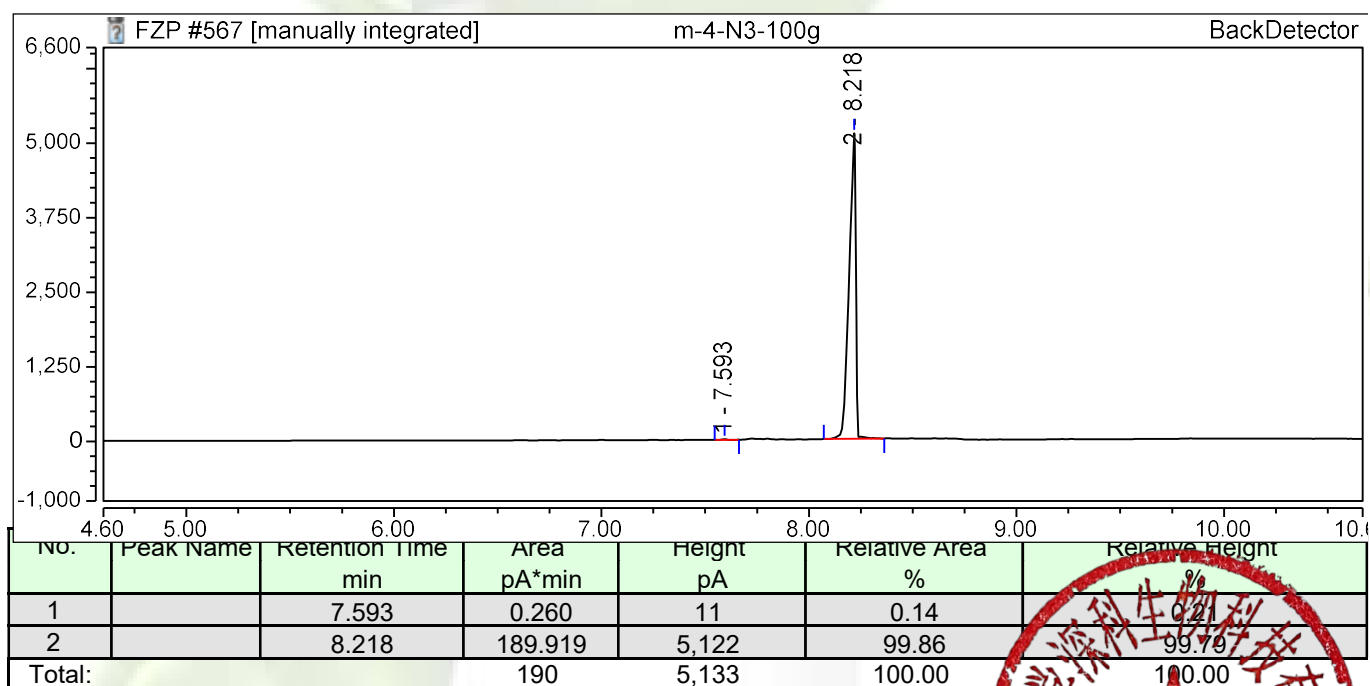

Mass Spectrum

Spectral plot could not be created.

No spectra selected.

