


Peak Analysis

Injection Details					
Injection Name:	3.4 MPEG4-OH?			Run Time (min):	16.50
Vial Number:	25			Injection Volume:	1.00
Injection Type:	Calibration Standard				
Calibration Level:					
Instrument Method:	100 hold 2 min 25 per 280 hold 6 min				
Processing Method:	mjj-0426			Dilution Factor:	1.0000
Injection Date/Time:	04/Mar/24 10:51			Sample Weight:	1.0000

Chromatogram

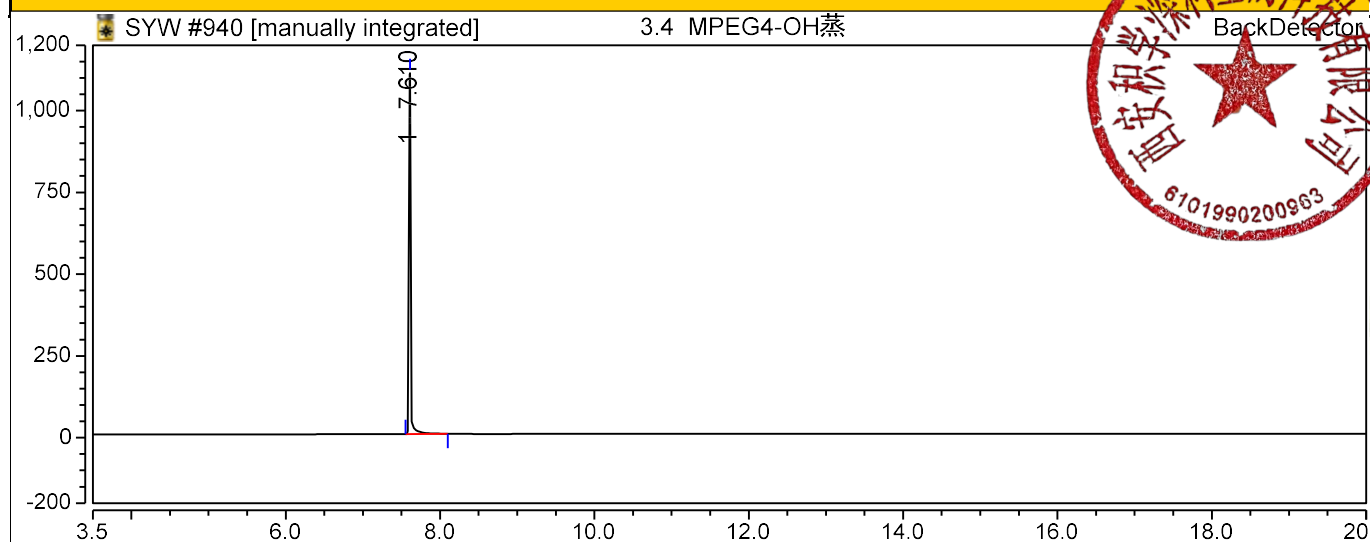

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %
1		7.610	27.861	1,103	100.00	100.00
Total:		28	1,103	100.00	100.00	100.00