


Chromatogram and Results

Injection Details

Injection Name:	NH2-P4-COOtBu-1-	Run Time (min):	12.50
Vial Number:	94	Injection Volume:	2.00
Injection Type:	Unknown	Channel:	BackDetector
Calibration Level:		Wavelength:	n.a.
Instrument Method:	80 hold 2 min 20 per 280 hold 2 min - Copy	Bandwidth:	n.a.
Processing Method:	Basic Quantitative(3)	Dilution Factor:	1.0000
Injection Date/Time:	23/Aug/24 11:37	Sample Weight:	1.0000

Chromatogram

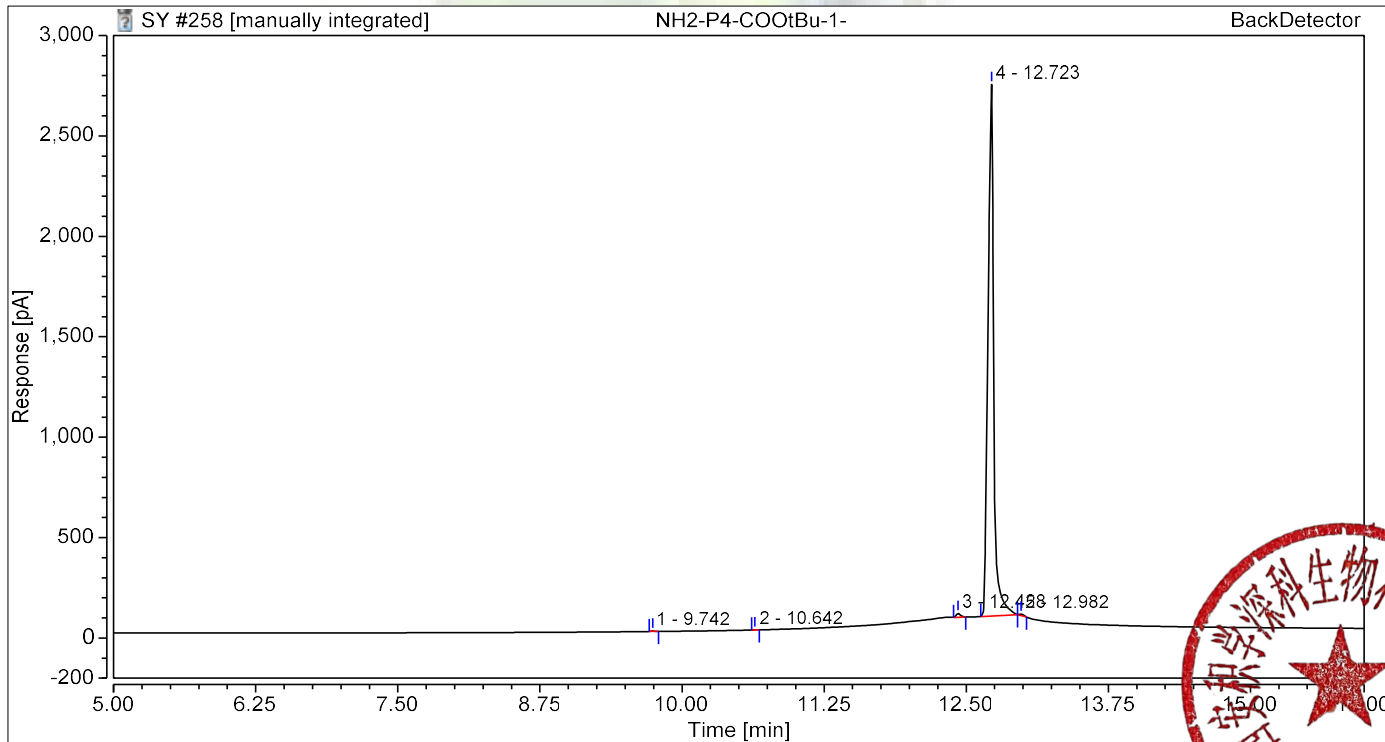

Integration Results

No.	Peak Name	Retention Time min	Area pA*min	Height pA	Relative Area %	Relative Height %	Amount n.a.
1		9.742	0.081	1.990	0.05	0.07	n.a.
2		10.642	0.046	1.448	0.03	0.05	n.a.
3		12.428	0.808	19.877	0.52	0.74	n.a.
4		12.723	153.893	2646.447	99.18	98.85	n.a.
5		12.982	0.332	7.350	0.21	0.27	n.a.
Total:			155.160	2677.113	100.00	100.00	